


MICROFILMED

FILED  
 GREENVILLE CO. S.C.  
 Oct 16 3 54 PM '80  
 BONNIE S. TANKERSLEY  
 R.M.C.

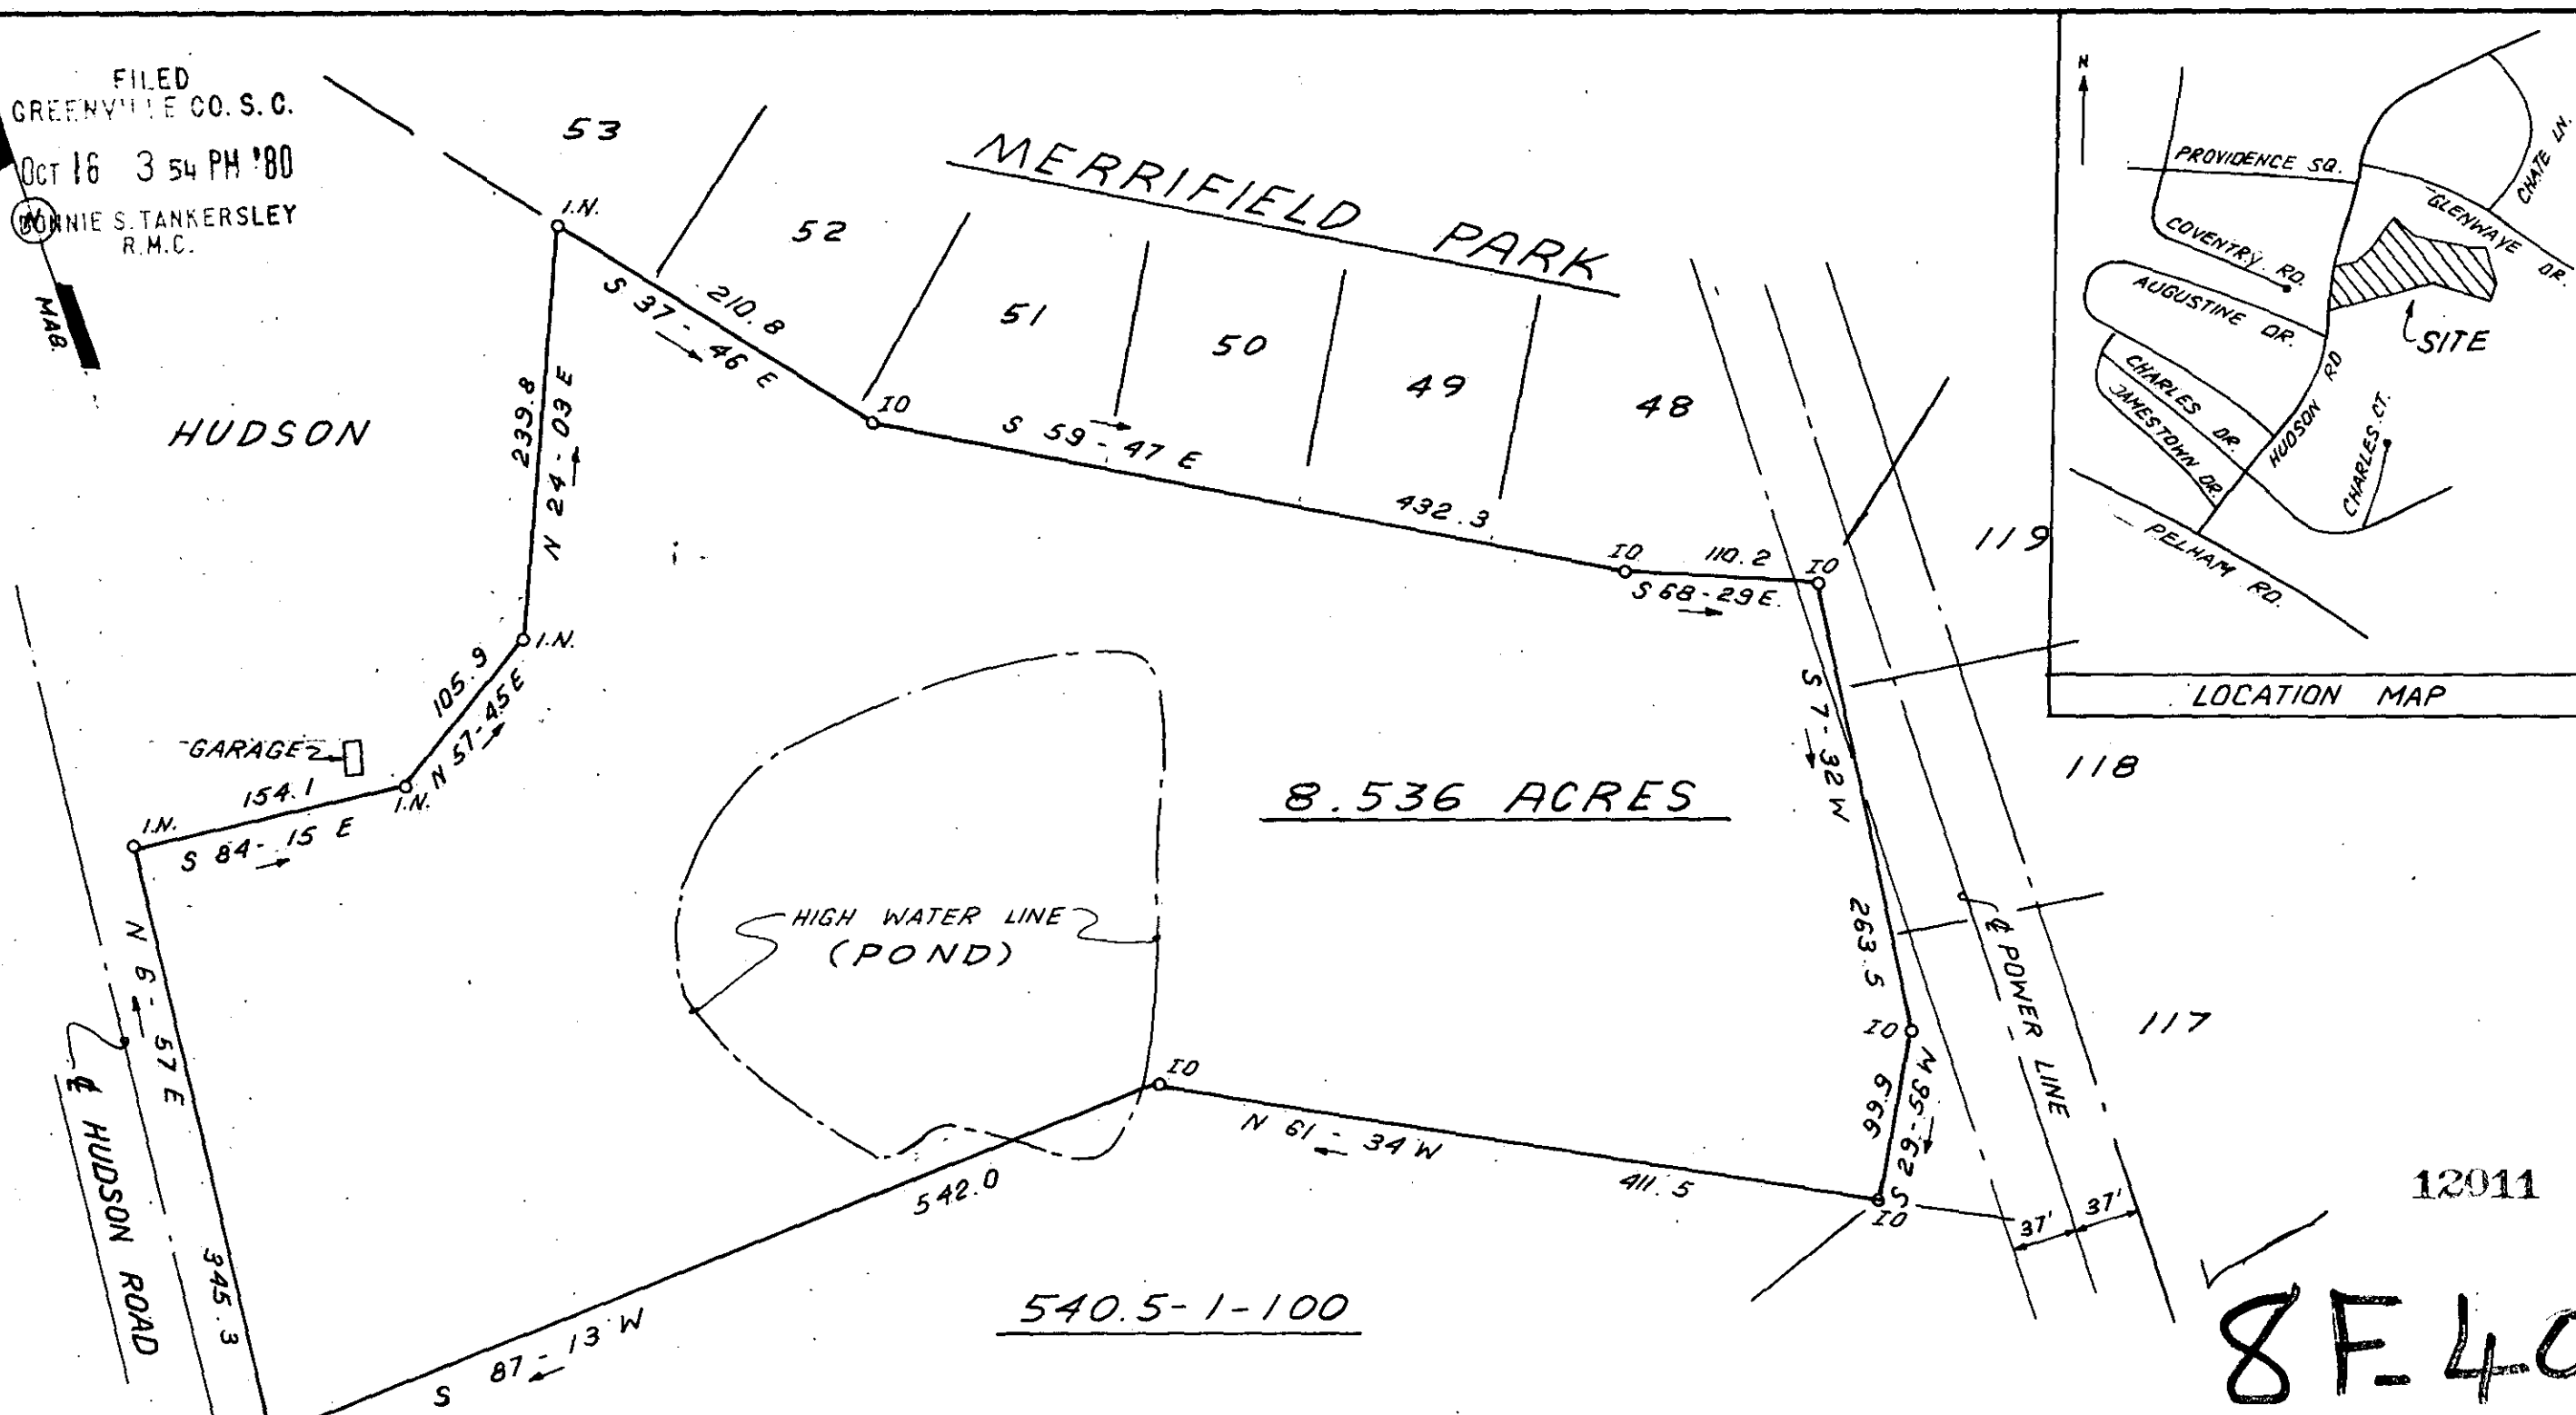

I hereby certify that the ratio of precision of the field survey is 1/5,000 as shown hereon and the area was determined by DMD Method.

*James R. Freeland*  
 James R. Freeland RLS & PE 4781



STATE OF SOUTH CAROLINA  
 GREENVILLE COUNTY

**SURVEY FOR**  
**KENNETH BOLT**

FREELAND & ASSOCIATES  
 Engineers • Land Surveyors  
 GREENVILLE, S.C.

SURVEY	L.T.
DRAWN	B.R.
CHECK	M.C.
SCALE	1" = 100'
DATE	SEPT. 29.80
DWG. NO.	5721

FOOTING OF 16.80 1166

5.000

PART BLK. BK. 540.5-1-99

8E.40